

Enhancing Precision in Robot-Assisted Surgery with Laser Interstitial Thermal Therapy

Carlos E. Marquez^{*1}, Elena Alvarez², João Pereira³

¹Instituto Politécnico Nacional, Mexico City, Mexico.

²Universidad de Buenos Aires, Buenos Aires, Argentina.

³Instituto Superior Técnico, Universidade de Lisboa, Lisbon, Portugal.

ABSTRACT

The performance of the minimally invasive surgery (MIS) is enhanced by new Robotic surgical assistants (RSAs) because of the many advantages including small incisions, decreased blood loss, less pain, quicker heating time and the ability to pinpoint locations very precisely.

In order to maximize therapeutic effects of the LITT (Laser interstitial thermal therapy) while minimizing side effects, thermal sensors need to be installed at the border between healthy and tumorous tissues. These thermal switches will send a signal to stop the heat process as soon as the temperature is exceeding a trigger. A mathematical formulation and a procedure is proposed that will help the physician prioritize the dosimetry locations and provide a safe dose per location. Such procedure which define the laser power distribution and the ablation position can be used for robot-assisted surgery. Such smart procedure will use a tissue damage prediction tool and bang-bang switch at the edges between healthy and unhealthy tissue to prevent side effect (laser ablation of the healthy tissue).

We used a system on chip to control the robotic arm and laser led in order to proceed with the automatic LITT procedure.

KEYWORDS: Laser Interstitial Thermal Therapy, thermal damage, brain cancer, bio heat transfer simulation, Thermal sensor, minimally invasive surgery, Robotic surgical assistants, Robotic arm, Raspberry Pi B+, Matlab, Comsol.

INTRODUCTION

The brain tumor tissue is modelled as a 3D domain with a structure of spheres after the laser ablation. Figure 1 shows the laser ablation sphere deformation formed during the ablation. In [Bla00] there is a demo of the NeuroBlate system laser delivery Probe. In this paper, the form of the deformation caused by the laser ablation is assumed to be as a sphere. The volume of the sphere will be defined during the simulation with respect to the temperature limit at the border between healthy and tumor tissues.

Each sphere represents the volume deformation of the tissue caused by a laser ablation of its sphere volume. Any sphere ablation will be represented with a sphere volume, sphere radius, laser power distribution through a time limit.

Since the tumor tissue is surrounded at the edge with thermal sensors, so they will not exceed a temperature limit, each sphere ablation assigned to the structure should verify this side effect constraint.

The laser ablation process is defined in the following steps:

- A. Assignment of the laser ablation point with spheres structure. The sphere ablation shouldn't have any side effect.
- B. An automatic ablation process will visit the structure within certain order and place the laser led at the center of the structure and proceed with the laser ablation of the spheres attached.

We defined the following thermal and optical properties for the brain tissue: conductivity, density, specific heat, diffusivity, relative permeability and electrical conductivity. The results will be the thermal distribution of the temperature and the volume of tissues damaged with the thermal switches [MHA17]. These results will be used to plan the dosimetry.

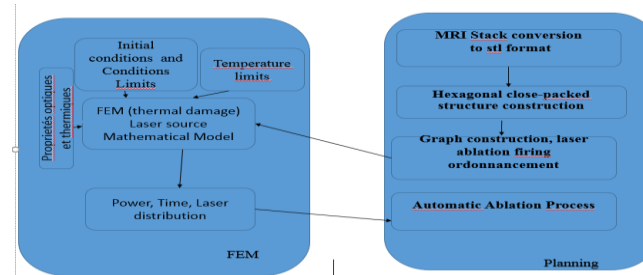


Figure 1. System Overview. The Planner relies on the FEM simulator. At each laser firing point, the planner will call the FEM.

The system has two modules as described fellow (figure 1.):

Planner.

First convert the MRI Stack to stl format, then the algorithm with construct the firing graph, and generate the laser ablation firing order. For each firing step call the FEM.

FEM.

Simulation software is used to simulate the mathematical model which use thermal conduction based on Fourier's law and constant blood perfusion. Predecting the results in term of volume damage to the tissu will improve the health care system. This module will send back the laser distrubution power so that no side effect will occurs.

Robotic Arm.

The robotic arm will receive the laser power distribution and the coodinate of the laser ablation point. Then put the laser led at the specified point and fire with the respect of the distribution during the specified time.

As stated in [SAC01], the planning process is divided into three steps :

- The selection of the number of beams and the direction from which to focus the laser ablation on the patient tumor tissue (geometry problem or beam angle optimization problem),
- The selection of intensity patterns for the directions selected in Phase 1 (intensity problem or fluence map optim,ization problem), and
- The selection de a delivery sequence that efficiently administers the treatment (realization problem or segmentation problem).

GENERAL MATHEMATICAL FORMULATION

The following paragraphs will specify the mathematical formulation of the automatic LITT, the description of the hexagonal close-packed structure, the graph contruction and the algorithm for the automatic ablation process.

Mathematical formulation of the Automatic LITT.

Let us assume that the laser beams of power $p = 1, \dots, n$ are available for a treatment and that each laser beam is fired on the tumor tissue to form a sphere with radium $r = 1, \dots, f$ at a specific point P with coordinates (x, y, z) with an angle $\alpha = 1, \dots, a$ to the z axis and within an exposition time $t = 1, \dots, m$ to kill the tissue in the volume of that sphere.

We denote $D_{(x,y,z),\alpha,p,r,t}$ the dose deposited at Point P with coordinate (x, y, z) , with an angle α , and with an exposition time of t .

We assume that there is a process which will divide the stl tissue format to as many as box. Then for ecah one we will execute the following automatic LITT procedure.

The tissue brain geometry is represented as a box of D_x mm wight by D_y mm length by D_z mm height , as shown in Figure 2. The tissue is then heated up to t minutes by a P Watt laser heat source. The initial temperature of the brain tissue is 37 degC.

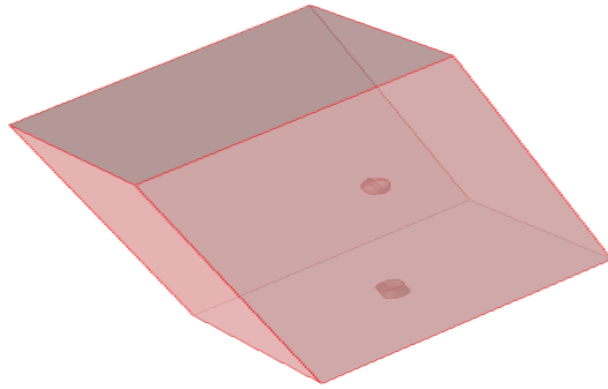


Figure 2. The tissue brain geometry is represented as a box.

We will represent the laser ablation point by a seven component vector :

$$(x_i, y_i, z_i, p_i, t_i, \alpha_i, V_i) \quad (1)$$

Where x_i, y_i, z_i represente the three dimentional cordinates, P_i is the power, t_i is the time, α is the angle and V_i is the binary variable between points that correspond to a new laser ablation entry from another.

$V_i = 1$, for any new laser ablation entry.
 $V_i = 0$, else.

Rule 1. Belonging to the same axle tire:

Whenever the point $x_2, y_2, z_2, P_2, t_2, \alpha_2, v_2$ belong to the same entry laser ablation point as $x_1, y_1, z_1, P_1, t_1, \alpha_1, v_1$ then one must have $(x_2, y_2) = (x_1, y_1)$, furthermore the coordinate of the entry point in the two dimensions, then z_2 mujst be LESS z_1 and $Z_2=0$.

Si $x_1 = x_2$ et $y_1 = y_2$ alors $z_2 < z_1$ et $V_2 = 0$ (2)

Rule 2. X 1 is the smallest of the x-axis coordinate.

We number the ablation point in such a way that x_i is the smallest x coordinate. Forthermore, we made the assumption that the ablation points are numbered in the increasing order of the x coordinate.

$$x_{i+1} \geq x_i \text{ is always true.} \quad (3)$$

Condition 1. Limit size of the tissue in axis x.

$$x_{i+1} - x_i \leq V_{i+1} D_x \quad (4)$$

Observation. If the $(i+1)$ th point correspond to a new entry (X_{i+1} Greater than X_i) then the Y coordinate of this point is free.

There is not necessarily $y_{i+1} \geq y_i$

$$\text{Si } x_{i+1} > x_i \text{ alors } y_{i+1} \text{ est libre} \quad (5)$$

Rule 3.

$$1. \text{ Si } x_{i+1} = x_i \text{ alors } y_{i+1} > y_i \quad (6)$$

$$2. \text{ Si } D_{i+1} = 0 \text{ alors } y_{i+1} > y_i \quad (7)$$

$$3. \quad y_i - y_{i+1} \leq D_{i+1} D_y \quad (8)$$

$$\text{Si } D_{i+1} = 1 \text{ alors } y_i - y_{i+1} \leq D_y \quad (9)$$

$$\text{Si } D_{i+1} = 0 \text{ alors } y_i - y_{i+1} \leq 0 \quad (10)$$

Condition 2 Belonging to the same axis shooting.

on sait que si $V_{i+1} = 0$ alors

$$\text{Si } z_{i+1} < z_i \text{ alors } z_{i+1} - z_i \leq v_{i+1} D_z \quad (11)$$

Condition 3.

$$y_i - y_{i+1} \leq v_{i+1} D_y$$

Et

$$y_{i+1} - y_i \leq v_{i+1} D_y \quad (12)$$

$$\text{Si } V_{i+1} = 0 \text{ alors } y_i > y_{i+1} \quad (13)$$

Condition 5. Total covering the Tumor tissue:

For any volume v of the Tumor Tissue, v should be part of at least one or many VD within the total Tumor Tissue.

Constraint of coverage, case of the spherical approximation.

Soit le centre du sphere (x_i, y_i, z_i, r) et soit le tir $(x_i, y_i, z_i, p_i, t_i, \alpha_i)$

A la question suivante: ce point (x, y, z) est brule?

$$(x_l - x_i)^2 + (y_l - y_i)^2 + (z_l - (z_i + r))^2 \leq r^2 + (1 - w_{il}) K$$

$$k = D_x^2 + D_y^2 + D_z^2$$

La contrainte de couverture est:

On a $\sum_{i \in I} w_{il} \geq 1$ quel que soit $l \in T$

Avec $w_{il} = 1$ si le voxel l est brule par le tir i

Avec $w_{il} = 0$ sinon.

Covering cubes constraint of coverage, case of the cubic approximation.

Cube inscrit dans la sphere et pointer en (x_i, y_i, z_i)

(x, y, z) avec $x \in (x_i - r, x_i + r)$ et $y \in (y_i - r, y_i + r)$ et $z \in (z_i, z_i + 2r)$

Soit $\Delta_x = |x - x_i|$ alors $\Delta_x \geq x - x_i$ et $\Delta_x \geq x_i - x$

Soit $\Delta_y = |y - y_i|$ alors $\Delta_y \geq y - y_i$ et $\Delta_y \geq y_i - y$

Soit $\Delta_z = |z - (z_i + r)|$ alors $\Delta_z \geq z - z_i - r$ et $\Delta_z \geq z_i + r - z$

Si $\Delta_x + \Delta_y + \Delta_z \leq r_i$ alors (x, y, z) appartient a un cube.

La contrainte de couverture de cube est

$$\Delta_{x_l} + \Delta_{y_l} + \Delta_{z_l} \leq r + (1 - w_{il}) K$$

Condition 6. Side effect constraint:

At each laser ablation point, and when firing the laser, there should be no violation at the thermal switches located at the edge points.

For each thermal switch TS:

$$\forall t, Temp(Ts) \leq Tlimit \quad (14)$$

The objective function is to minimise the number of laser ablations:

$$\min \sum_{i=1}^n u_i + \beta \sum_{i=1}^n v_i \quad (15)$$

U is the number of reprints, and V the number of axes of tires, and B is a parameter.

Definition of the Thermal damage:

We used the first order Arrhenius equation to compute the damage integral [MHA17]:

$$\Omega(t) = \ln \frac{C_0}{C_{UD}(t)} = \int A \exp \left[-\frac{E_a}{RT(t)} \right] dt \quad (16)$$

where C_0 is the original concentration of undamaged cells, C_{UD} is the concentration of the remaining living cells after time t, the treatment time, A is the frequency factor, E_a is the activation energy and R is the universal gas constant. ($R=8.314 \text{ J mol}^{-1} \text{ K}^{-1}$).

A damage integral of $\Omega = 1$, corresponds to 63% percent probability of cell death, and damage integral of $\Omega = 4.6$, corresponds to 99% percent probability of cell death at a specific point.

DESCRIPTION OF THE AUTOMATIC ABLATION PROCESS

Either the number of division on nx x axis.

$NX = x/a$.

The same way, we can calculate Ny and Nz.

Then a plan of treatment with (Nx.Ny.Nz) cubes. With Nx.Ny.Nz is equal the number of reprints.

If we vary the edge has, we'll have another tire plan.

Among the plans drawn, you evaluate them based on the side effect the objective function and offer the best.

To the edges of the fabric, we will propose a refinement.

To optimize the number of ablation, a combination of Side Fire and Full fire will be proposed as follow:

When the firing point is in the center of the Tissue, The NeuroBlate diffusing laser (Full Fire) is designed to provide fast, volumetric ablation in a concentric zone of hyperthermia.

While the firing point is near the edges of the Tissue, The NeuroBlate directional laser (SideFire) is the preferred tool for contoured ablation of targets while sparing adjacent healthy tissue.

All full Fire and Side Fire have to verify the side effect constraints.

MATERIALS AND METHODS

A. Modeling in COMSOL Multiphysics

A.1. Heat distribution and damage estimation.

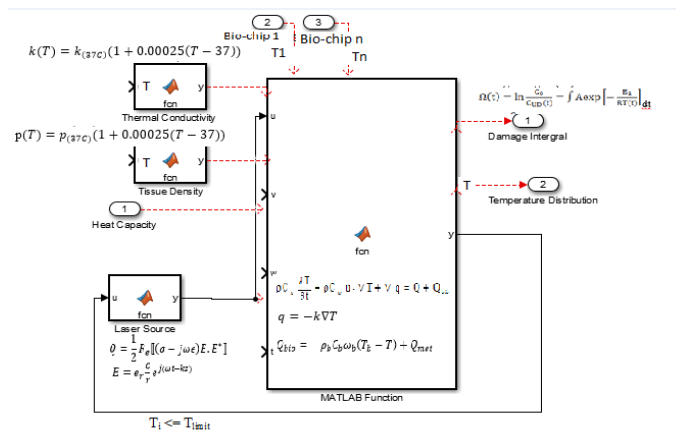


Figure 3. Validation process and damage estimation tool.

In [MHA17] a validation process was done between mathematical modelisation and many real data. The result was to propose an estimation tool for the tissue damage during the laser ablation. This tool can be used by physician to predict tissue damage and plan the dosimetry. Figure 3 shows the process of this validation which include the variation of the thermal conductivity and tissue density, the edge temperature detection and their feedback in case they exceed a temperature limit.

A.2 Bang-bang Controller

In [BAH17], visual thermal sensors were implemented at the border between healthy and tumorous brain tissues. Events interface to control the heating process, by either allowing or stopping the source function depending on a temperature limit. As soon as the thermal controller reaches the temperature limit at the border, it will send a signal to stop the heating process immediately.

B Matlab, Comsol simulation and robotic arm.

B1. Matlab codes to access the Comsol simulation.

Loading a comsol model at the matlab prompt:

```
model = mphload('busbar.mph');
```

Then working with the geometry, working with meshes, modeling physics, executing the comsol program within matlab.

A matlab loop will go through the geometry and call Comsol simulation using thermal switches at the edges of the tumor tissue. If the power proposed does not permit the temperature to exceed the temperature limit, the robotic arm can proceed with the laser ablation.

B.2 Matlab codes to control the laser LED through a Raspberry PI B+

The following program will check the temperature at the edges, if temperature limit is exceeded, the program will display 'do not proceed' else the program will display 'Please proceed with the laser ablation.'

```
clear;
mypi=raspi;%
filename=fullfile('C:\users\mhamed\desktop\max-op2.txt');
fid = fopen(filename, 'r') ;
%Opensourcefile.
fori=1:8
fgetl(fid) ;
%
Read/discardline.
end;
buffer=fread(fid, Inf) ;
%Readrestofthefile.
fclose(fid)
fid = fopen('C:\users\mhamed\desktop\max-
output.txt', 'w') ; % Open destination file.
fwrite(fid, buffer) ;
% Save to file.
fclose(fid) ;
%
filename = fullfile('C:\users\mhamed\desktop\max-output.txt');
T1 = readtable(filename);
C = table2cell(T1);
C
max([C{:, :}])
if any([C{:, :}] > 37)
    disp('There is at least one value above the limit. Please do not proceed !!!')
else
    disp('All values are below the limit. Please Proceed.')
end
%
%
filename = fullfile('C:\users\mhamed\desktop\donne-binaire.txt');
fid = fopen(filename, 'r') ;
```

```
% Open source file.
for i=1:8
    fgetl(fid) ;
% Read/discard line.
end;
buffer = fread(fid, Inf) ;
% Read rest of the file.
fclose(fid)
fid = fopen('C:\users\mhamed\desktop\donne-output.txt', 'w') ; % Open destination file.
fwrite(fid, buffer) ;
% Save to file.
fclose(fid) ;
%
filename = fullfile('C:\users\mhamed\desktop\donne-output.txt');
T = readtable(filename);
for i=1:30
    writeDigitalPin(mypi, 25,T(i,2));
    pause(0.03);
end;
```

B3. Matlab codes to control the Robotic Arm.

To control the 6-axis robotic arm, there are manual and an automatic option:

Option 1 is to use the March 3 CNC controller software to send the coordinates of the firing points to the robotic arm. The MATLAB script will execute the COMSOL program, then via the CNC controller, we will control the robotic arm using the Mach 3 program.

Option 2 is to automatically control the robotic arm by using ABB robot Studio. Selecting the robot and tool to simulate the robotic arm and led. The Rapid program includes the path (set of positions) received from the Matlab. The command MoveL with data from the file as positions with move to different positions in order to proceed with the laser ablation. The syntax of the Move l is MoveL RelTool (p1, 0, 0, 100), v100, fine, tool1; the robot is moved to a position that is 100 mm from p1 in the z direction of the tool.

CONCLUSION

In this paper, a framework for automatic laser ablation was proposed, which include all steps from the calculation of the temperature distribution and tissu dammage, the control of the temperature at the edges, then the safe automatic ablataion process with no side effects. Next step will be the implentation of the whole framework.

REFERENCES

- [1] [SAC01] Sachin, Ron Alterovitz, Automated Tissue Retraction for Robot-Assisted Surgical Surgical Procedures, Department of Computer Science, University of North Carolina at Chapel Hill, USA.
- [2] [BAH17]. Mhamed Nour, Mohammed Bougataya Ahmed Lakhssassi, , Using Virtual Bang-Bang Controllers to Optimize Treatment of Brain Tumors, 1st International Conference on Advanced Research (IACR 2017) Manama, Bahrein, Jan 25-26, 2016.
- [3] [MHA17] Mhamed Nour, Aziz Oukaira, Mohammed Bougataya, and Ahmed Lakhssassi, "Thermal Damage Modeling Analysis and Validation during Treatment of Tissue Tumors," International Journal of Pharma Medicine and Biological Sciences, Vol. 6, No. 4, pp. 98-104, October 2017. doi: 10.18178/ijpmbs.6.4.98-104
- [4] [Matlab] Matlab numeral computing. Tutorialspoint.